

Continuous Radon Monitor

Model Number: 1029

Calibration Date: 06/01/2007

Monitor Time: 2/14/2008 13:13

Serial Number: 4974617

CF: 2.96, 2.79

Inspector Information

Company Name

Phone Number: 321-123-4567

Customer Information

Atmospheric Condition: NA

Structure Type: NA

Monitor Location: NA

Site & Condition

Wind: NA

Year Built: NA

SqFt: NA

Test Summary

Start Time: 02/13/2008 17:04

End Time: 02/14/2008 13:04


Measurement Interval (hr): 0.5

Elapsed Time: 0 Days 20 hrs

Overall Avg: 1.811E4 Bq/m³

EPA Avg: 1.894E4 Bq/m³

Continuous Radon Monitor

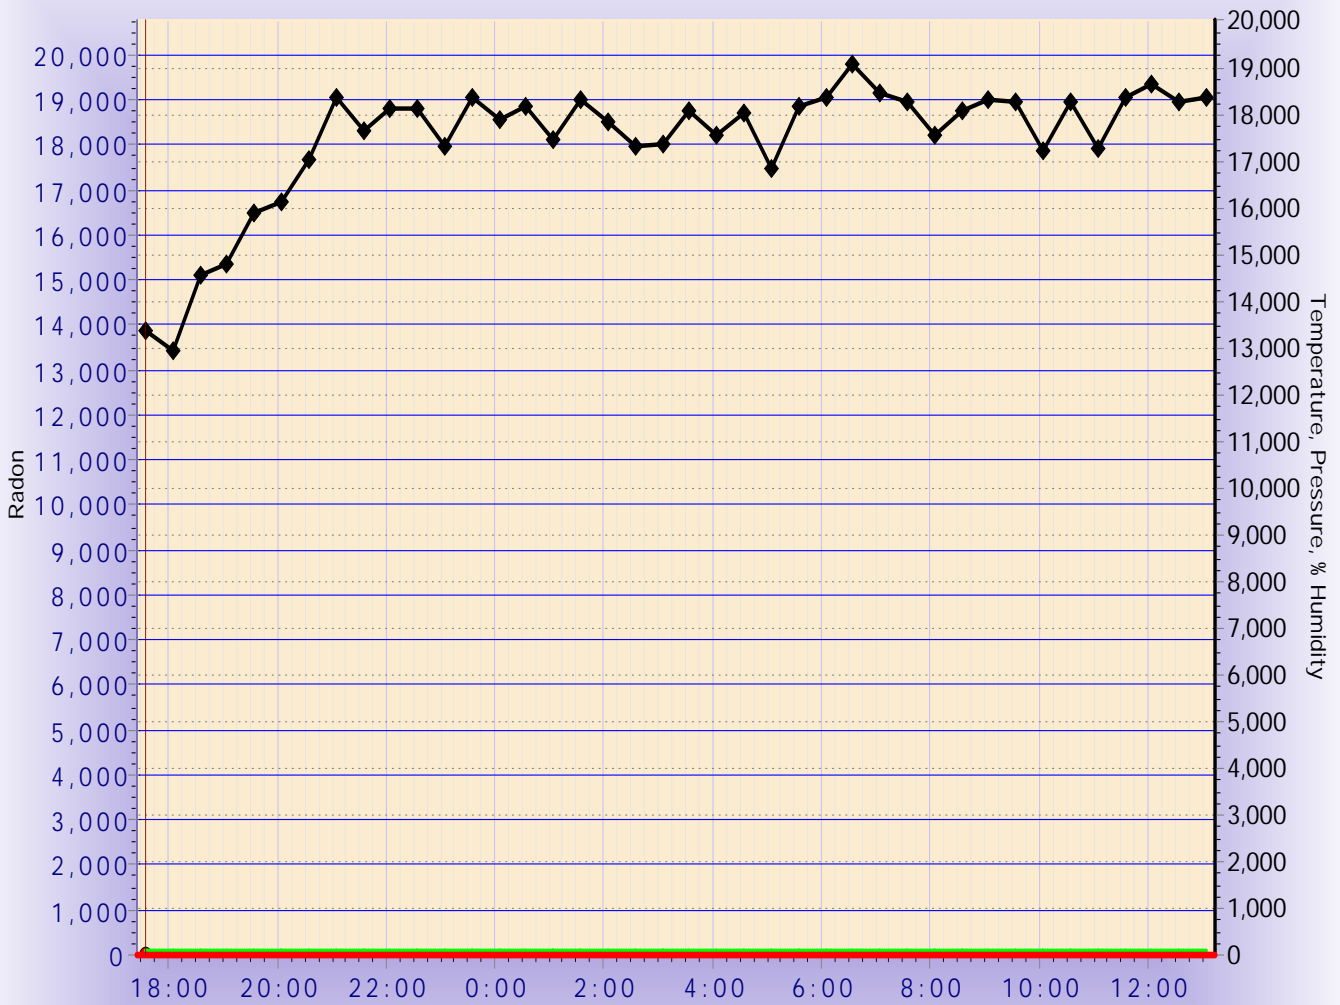

◆ Radon Bq/m³ ● Motion Errors — Temp C — Rel % Humidity
— Press kPa

***** 02/ 13/ 2008 *****

Time	Counts Bq/ M3	Temp C	Pressure Pa	Humidity	Flags
17:34	13870.0	21.3	1015.2	31.8	M
18:04	13433.3	20.9	1015.8	29.0	
18:34	15107.2	20.7	1015.2	27.1	
19:04	15342.5	20.6	1015.2	26.2	
19:34	16501.3	20.5	1015.2	25.3	
20:04	16731.3	20.5	1015.8	24.6	
20:34	17643.4	20.5	1015.8	24.2	
21:04	19050.5	20.6	1015.2	23.5	
21:34	18327.7	20.5	1016.2	23.1	
22:04	18779.7	20.6	1015.8	22.6	
22:34	18811.9	20.6	1014.8	22.4	
23:04	17939.4	20.5	1015.8	22.1	
23:34	19026.0	20.4	1015.8	22.0	

***** 02/ 14/ 2008 *****

Time	Counts Bq/ M3	Temp C	Pressure Pa	Humidity	Flags
00:04	18539.3	20.3	1015.8	21.5	
00:34	18832.6	20.3	1015.8	21.4	
01:04	18125.5	20.1	1015.2	21.2	
01:34	19023.2	20.1	1016.5	21.1	
02:04	18497.2	20.0	1015.5	20.8	
02:34	17939.2	19.9	1014.5	20.7	
03:04	17987.8	19.8	1014.8	20.4	
03:34	18763.9	19.6	1016.2	20.5	
04:04	18233.5	19.6	1016.2	20.1	
04:34	18725.6	19.5	1015.8	20.1	
05:04	17480.3	19.3	1015.5	20.1	
05:34	18828.2	19.2	1015.8	20.0	
06:04	19040.3	19.1	1016.5	19.8	
06:34	19785.8	19.1	1016.5	19.7	
07:04	19141.2	18.9	1017.2	19.6	
07:34	18941.7	18.8	1017.2	19.5	
08:04	18196.2	18.7	1017.2	19.5	
08:34	18752.9	18.6	1017.5	19.3	
09:04	19008.1	18.6	1017.5	19.3	
09:34	18943.5	18.5	1015.8	19.2	
10:04	17862.6	18.3	1015.8	19.0	
10:34	18942.0	18.3	1016.2	19.0	
11:04	17893.7	18.2	1017.2	18.9	
11:34	19031.6	18.2	1016.5	18.9	
12:04	19320.0	18.1	1014.8	18.7	
12:34	18955.3	18.1	1013.8	18.7	
13:04	19038.8	18.0	1013.1	18.6	

Error Flags:

M Motion:

Inspector Signature _____

PC Software Version: 2.0.0.0

Embedded Software Version: 104